NOTES:
1. SEE STRATUS INSTALLATION INSTRUCTIONS FOR DETAILS ON MOUNTING COMPONENTS AND ROUGH-IN LOCATION REQUIREMENTS. REFERENCE DRAWING 5830-A0-0020 FOR STANDARD PARTS ASSEMBLY.
2. WIRING WILL BE FIELD CONNECTED TO JUNCTION BOXES (LOCATED ON ROUGH-IN TEMPLATE) DURING INSTALLATION.
3. 150 WATT TRANSFORMER FOR BRAKES WILL BE PROVIDED ON THE ROUGH-IN TEMPLATE AND WIRED TO THE EMER POWER JUNCTION BOX.

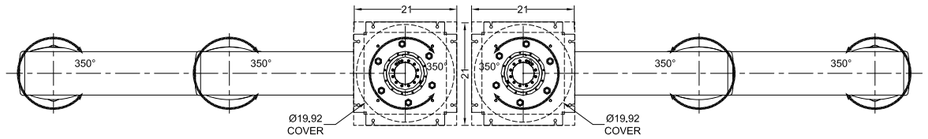

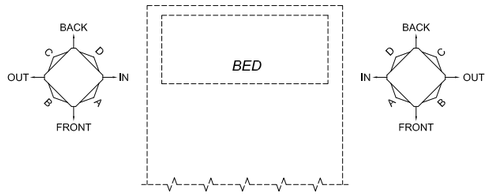

SEPARATE MOUNTING PLATES ARE PROVIDED FOR INDEPENDENT MOUNTING. POSITIONING WILL BE BASED ON THE 2x2 CEILING GRID WITH THE MINIMUM OFFSET BEING 24" BETWEEN CENTERLINES UNLESS OTHERWISE SPECIFIED. SERVICE CONNECTIONS WILL BE ON THE THREE OPEN SIDES ONLY.

___ *REQ'D:* ___ *AS SHOWN*
___ *OPPOSITE*

CORRIDOR

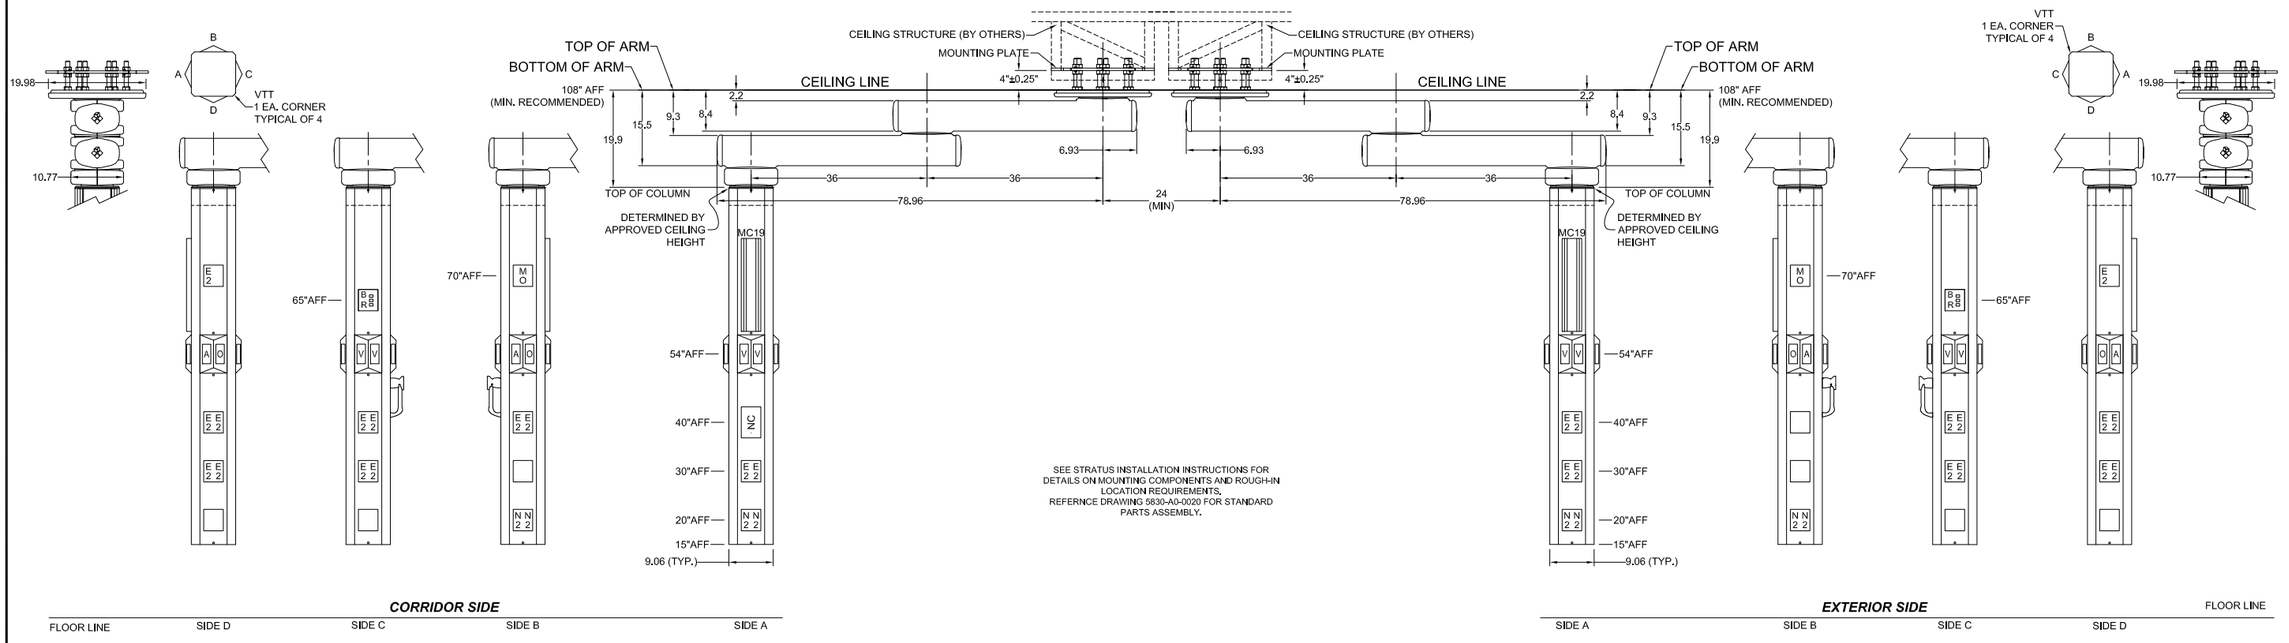

SEE STRATUS INSTALLATION INSTRUCTIONS FOR DETAILS ON MOUNTING COMPONENTS AND ROUGH-IN LOCATION REQUIREMENTS. REFERNCE DRAWING 5830-A0-0020 FOR STANDARD PARTS ASSEMBLY.

EXTERIOR SIDE

GENERAL SPECIFICATIONS:

ELECTRICAL		PLUMBING		FINISHES	
NORMAL POWER JUNCTION BOX:	J1	HOSE TUBING:	-		
EMERGENCY POWER JUNCTION BOX:	J2	OXYGEN SIZE (I.D.):	1/4"		
LIGHTING JUNCTION BOX:	J5	MEDICAL AIR SIZE (I.D.):	1/4"		
LV CONDUIT STUBS:	NC, DP	VACUUM SIZE (I.D.):	5/16"		
CONDUIT SIZE; LINE VOLTAGE:	1/2"				
CONDUIT SIZE; LOW VOLTAGE:	3/4"				
CONDUIT CONNECTORS:	STD. SET SCREW			PANEL COLOR:	POWDER COATED TO MATCH SURF.
WIRE TYPE:	THHN, STRANDED			TRIM & GAS PODS:	MATCH SURF.
WIRE SIZE:	12 AWG			EQUIPMENT MANAGEMENT:	ANODIZED ALUMINUM
GROUND WIRE COLOR:	GREEN			ELECTRICAL COVER PLANTES:	POWDER COATED TO MATCH SURF.

LEGEND:

REQ	SYM	DESCRIPTION	REQ	SYM	DESCRIPTION
4	O	OXYGEN OUTLET			
4	A	AIR OUTLET			
8	V	VACUUM OUTLET			
8	N2	DUPLEX RECEPTACLE, 8300 IVORY 20A, 125V, H.G., NORMAL POWER			
26	E2	DUPLEX RECEPTACLE, 8300 RED 20A, 125V, H.G., EMER. POWER			
1	NC	NURSE CALL PROVISION			
2	MO	MONITOR OUTPUT PROVISION			
2	MC19	MONITOR CHANNEL ONLY, 19" LENGTH			
2	BR	BRAKE RELEASE			
8	VTT	VERTICAL EQUIPMENT MOUNTING TRACK, TRIPLE			

ACCESSORIES NOT SHOWN (PER UNIT)

REQ	DESCRIPTION	REQ	DESCRIPTION
2	NON FUNCTIONING HANDLE FOR POSITIONING, ATTACHES TO VTT LEFT OF LED HANDLE		

MODULAR SERVICES COMPANY®
500 EAST BRITTON ROAD
OKLAHOMA CITY, OK 73114
www.modularservices.com

PROJECT
HOSPITAL
PROJECT
CITY, STATE

TOTAL QTY:	DUAL STRATUS® II, 5830 SERIES MODEL 5832-D	
X		
AS SHOWN: X	DRAWN BY: XXX	DRAWING # 4XXXX
OPPOSITE: X	DATE: XX/XX/XX	PROJECT #: XXXX / SALES ORDER #: XXXXX